


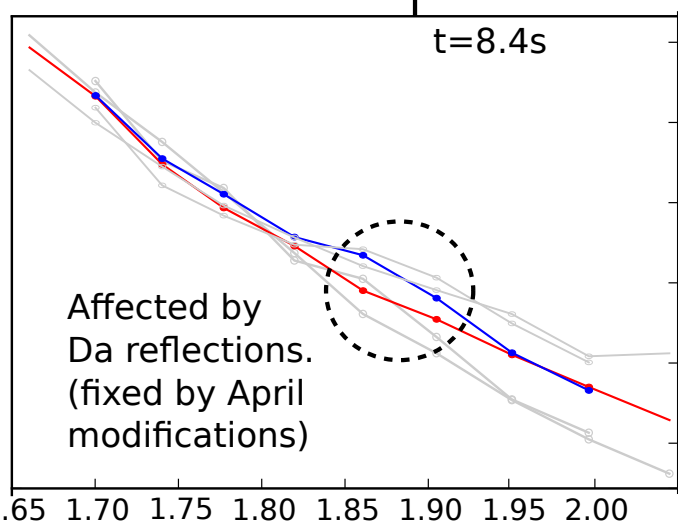


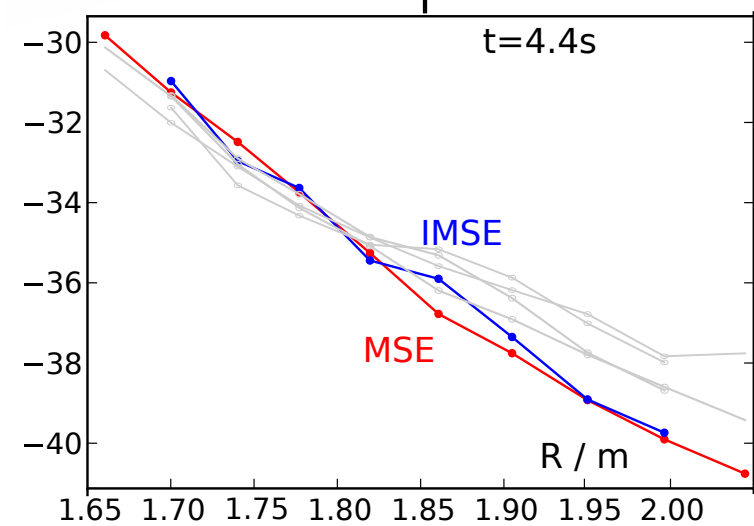

Direct MSE - IMSE comparison

To compare the IMSE/MSE systems directly, the same pulse was run the following week with the MSE system.



Temporal evolution agreement is very good, spatial agreement is reasonable and was improved recently. An unidentified offset of 1.1° is still required, but is constant for the whole image.